


MODEL 9000/5000/5000B
 Microbial Reduction of Bacillus subtilis



* **Tester:** Intertek ETL-Semko. **Test Scope:** Microbial Reduction. **Rate testing:** Test the ability of air cleaners to reduce the number of microorganisms injected into a closed room.
Standard and Test used: Intertek Non STD, Microbial Reduction Rate. **Test Organisms:** Bacillus subtilis (bacteria), were obtained from the US Department of Agriculture, Microbial and Bioprocessing Research Unit. **Date of test:** Dec.20, 2004. **Report No.** 3069236-02.

MODEL 9000S/5000S
 Microbial Reduction of Bacillus subtilis

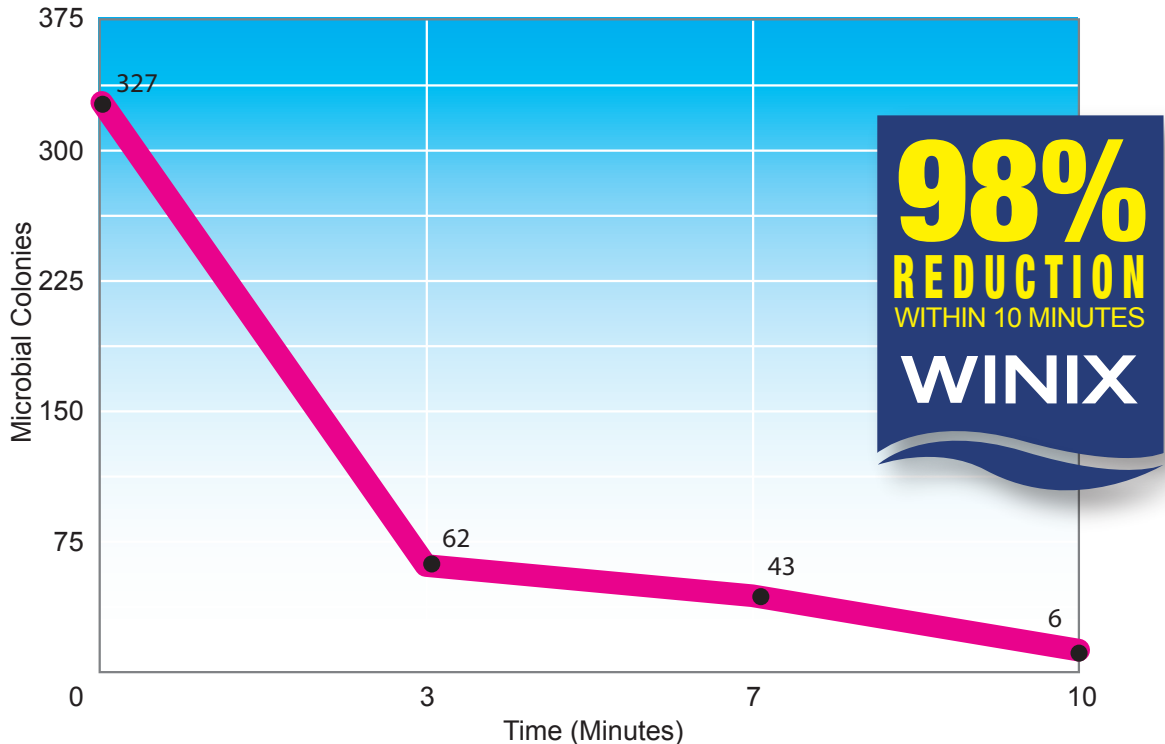

* **Tester:** Intertek ETL-Semko. **Test Scope:** Microbial Reduction. **Rate testing:** Test the ability of Air cleaners to reduce the number of microorganisms injected into a closed room,
Standard and Test used: Intertek Non STD, Microbial Reduction Rate. **Test Organisms:** Bacillus subtilis (bacteria), were obtained from the US department of Agriculture, Microbial and Bioprocessing Research Unit. **Date of test:** Dec.20, 2004. **Report No.** 3069236-02